

HiTrap IgM Purification HP

HiTrap™ IgM Purification HP is a 1-ml column designed for fast and efficient purification of monoclonal IgM from hybridoma cell cultures. The prepacked columns are easily connected to a syringe, peristaltic pump, or a chromatography system such as ÄKTAdesign™. With this column, IgM purification becomes a simple, one-step elution procedure.

Key characteristics of HiTrap IgM Purification HP columns include:

- Fast and easy purification of monoclonal IgM
- High purity with retained activity
- Convenient use

Medium characteristics

HiTrap IgM Purification HP columns are packed with a thiophilic adsorption medium with 2-mercaptopyridine coupled to Sepharose™ High Performance. Thiophilic adsorption is promoted by water-structuring salts. The interaction between protein and ligand has been suggested to result from a combined electron donating and accepting action of the ligand, or alternatively as a mixed mode hydrophilic-hydrophobic interaction.

The base matrix, Sepharose High Performance, has good flow properties as well as high physical and chemical stability. The main application of HiTrap IgM Purification HP is purification of IgM from hybridoma cell cultures.

Column characteristics

HiTrap columns are made of polypropylene, which is biocompatible with biomolecules. Top and bottom frits are manufactured from porous polyethylene. The columns are delivered with a stopper on the inlet and a snap-off end on the outlet.

The characteristics of HiTrap IgM Purification HP columns are shown in Table 1.



Fig 1. HiTrap IgM Purification HP 1-ml column.

Table 1. Characteristics of HiTrap IgM Purification HP columns

Column volume	1 ml
Column dimensions	0.7 × 2.5 cm
Ligand	2-mercaptopyridine
Ligand concentration	2 mg/ml medium
Binding capacity	5 mg human IgM/ml medium
Mean particle size	34 µm
Matrix	Highly cross-linked spherical agarose
Recommended flow rate	1 ml/min
Maximum flow rate ¹	4 ml/min
Maximum backpressure	3 bar (0.3 MPa)
pH stability ²	
Long term	3–11
Short term	2–13
Temperature stability	
Regular use	4°C to room temperature
Storage	4°C to 8°C
Storage buffer	20% ethanol

¹ Room temperature, aqueous buffers

² The ranges given are estimates based on our knowledge and experience. Please note the following: *pH stability, long term* refers to the pH interval where the medium is stable over a long period of time without adverse effects on its subsequent chromatographic performance. *pH stability, short term* refers to the pH interval for cleaning.



Fast and easy purification of IgM

Purifying IgM is a fast and easy procedure with HiTrap IgM Purification HP. Simply attach the column to the selected equipment, apply sample, wash, and then elute the bound IgM in a single step. See Figure 2 for an example of use with a syringe. Complete, easy to follow “step-by-step” instructions for fast start up and method optimization, together with recommendations for sample preparation, are included with the columns.

For large sample amounts, several columns can be easily connected in series. The columns cannot be opened and repacked.

Operation

As for all HiTrap columns, HiTrap IgM Purification HP is convenient to use. A set of connectors supplied with the column enables easy connection to a syringe, a peristaltic pump, or a liquid chromatography system.

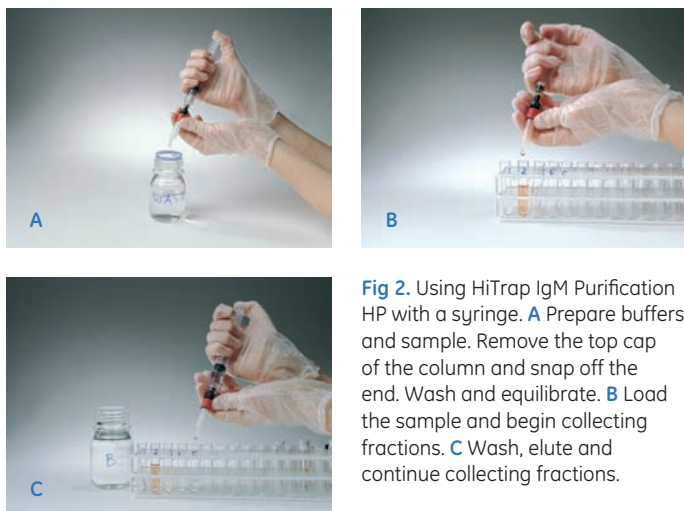


Fig 2. Using HiTrap IgM Purification HP with a syringe. **A** Prepare buffers and sample. Remove the top cap of the column and snap off the end. Wash and equilibrate. **B** Load the sample and begin collecting fractions. **C** Wash, elute and continue collecting fractions.

High purity

Results from the purification of monoclonal α -Shigella IgM from hybridoma cell culture supernatant show that the eluted IgM is more than 80% pure and retains its high activity (see Applications).

Applications

Monoclonal α -Shigella IgM from a hybridoma cell culture supernatant was purified on HiTrap IgM Purification HP. After sample loading the column was washed and IgM was eluted with sodium phosphate. Remaining impurities were eluted with 30% isopropanol (Fig 3).

Column: HiTrap IgM Purification HP 1 ml
 Sample: 75 ml of cell culture supernatant containing α -Shigella IgM, filtered through a 0.45 μ m filter
 Binding buffer: 20 mM sodium phosphate buffer, 0.5 M potassium sulphate, pH 7.5
 Elution buffer: 20 mM sodium phosphate buffer, pH 7.5
 Cleaning buffer: 20 mM sodium phosphate buffer, 30% isopropanol, pH 7.5
 Flow rate: 1 ml/min
 System: ÄKTApurifier™ 10S

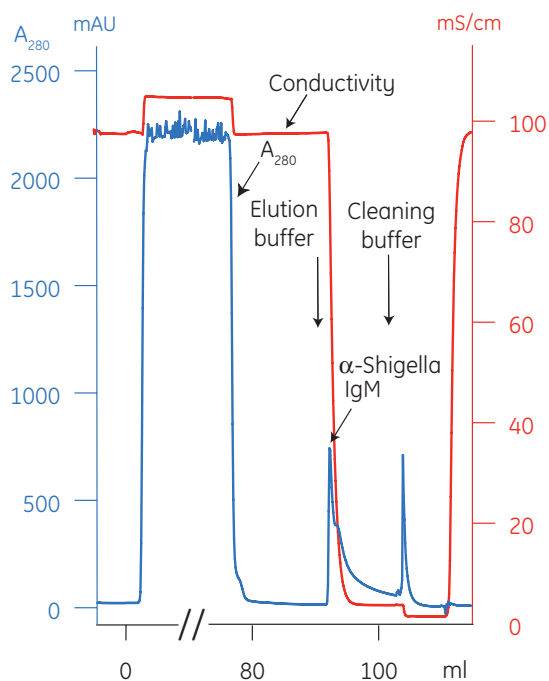


Fig 3. Purification of α -Shigella IgM on HiTrap IgM Purification HP.

ELISA detection of α -shigella IgM

Results from ELISA showed that active protein was eluted and that all IgM included in the large sample volume bound to the column, Table 2.


Table 2. Activity of α -Shigella IgM measured by ELISA

Sample	α -Shigella IgM conc. (mg/ml)	Volume (ml)	Recovery (%)
Cell culture supernatant	0.01	100	100
Flow-through pool, 0–90 ml	n.d. ¹	90	0
Flow-through pool, 90–100 ml	n.d.	10	0
Eluate	0.1–0.3	9	>100%
Cleaning eluate	approx. 0.1	1	approx. 10

¹ n.d. = not detectable

Determination of purity

The identity and purity of the eluted IgM fractions were measured by SDS-PAGE electrophoresis and by analytical gel filtration (see Figures 4a, 4b, and 5). The results show excellent purity, > 80%, of the collected IgM fractions.

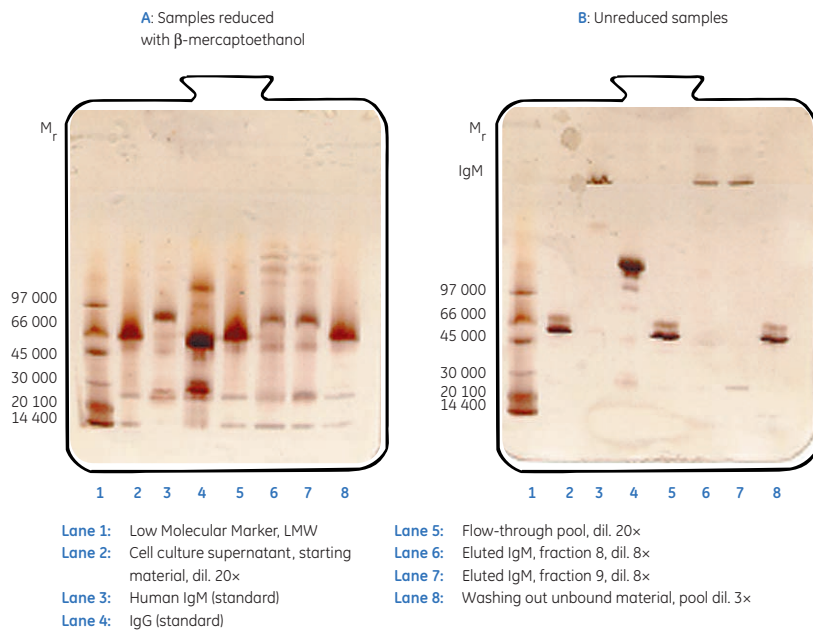

Column: Superdex™ 200, 10 × 300 mm
 Sample: 250 μ l of pooled α -Shigella IgM eluate from HiTrap IgM Purification HP
 Buffer: 20 mM sodium phosphate buffer, 0.15 M sodium chloride, pH 7.2
 Flow rate: 0.5 ml/min
 System: ÄKTApurifier 10S

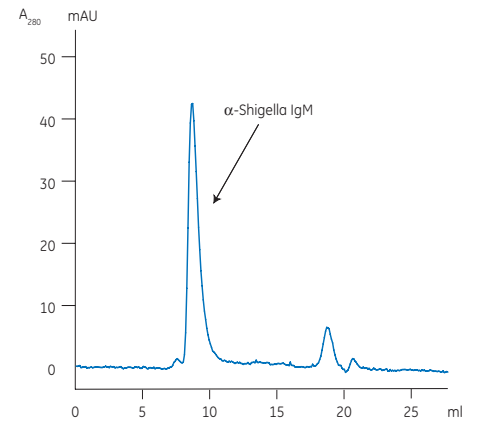


Fig 5. Gel filtration on Superdex 200, 10 × 300 mm column.

Fig 4. SDS-PAGE on PhastSystem™, using PhastGel™ 4–15, silver staining.

Table 3. Physio-chemical properties of human immunoglobulins

Immunoglobulin	Heavy chain	Light chain	Sedimentation coefficient	Mol. Wt (M_r)	M_r heavy chain	Carbohydrate content (%)	A_{280nm}	pI
IgG ₁	λ_1	κ, λ	7S	146 000	50 000	2–3	13.8	5.0–9.5
IgG ₂	λ_1	κ, λ	7S	146 000	50 000	2–3		5.0–8.5
IgG ₃	λ_1	κ, λ	7S	170 000	60 000	2–3		8.2–9.0
IgG ₄	λ_1	κ, λ	7S	146 000	50 000	2–3		5.0–6.0
IgM	μ	κ, λ	19S	900 000	68 000	12	12.5	5.1–7.8
IgA ₁	α_1	κ, λ	7S	160 000	56 000	7–11	13.4	5.2–6.6
IgA ₂	α_2	κ, λ	7S	160 000	52 000	7–11		5.2–6.6
IgA ₃	α_1, α_2	κ, λ	11S	370 000	52–56 000	11		4.7–6.2
IgD	δ	κ, λ	7S	184 000	68 000	12	17.0	–
IgE	ϵ	κ, λ	8S	190 000	72 000	12	15.3	–

Table 4. Physio-chemical properties of mouse immunoglobulins

Immunoglobulin	Heavy chain	Light chain	Sedimentation coefficient	Mol. Wt (M_r)	M_r heavy chain	Carbohydrate content (%)	pI
IgG ₁	λ_1	κ, λ	7S	150 000	50 000	2–3	7.0–8.5
IgG _{2a}	λ_{2a}	κ, λ	7S	150 000	50 000	2–3	6.5–7.5
IgG _{2b}	λ_{2b}	κ, λ	7S	150 000	50 000	2–3	5.5–7.0
IgG ₃	λ_3	κ, λ	7S	150 000	50 000	2–3	–
IgM	μ	κ, λ	19S	900 000	80 000	12	4.5–7.0
IgA	α	κ, λ	7S	170 000	70 000	7–11	4.0–7.0
IgD	δ	κ, λ	7S	180 000	68 000	12–14	–
IgE	ϵ	κ, λ	8S	190 000	80 000	12	–

Ordering information

Product	Quantity	Code No.
HiTrap IgM Purification HP	5 × 1 ml	17-5110-01

Related products	Quantity	Code No.
HiTrap Desalting	5 × 5 ml	17-1408-01
HiPrep™ 26/10 Desalting	1 × 53 ml	17-5087-01
HiPrep 26/10 Desalting	4 × 53 ml	17-5087-02

Accessories	Quantity	Code No.
1/16" male/Luer female ¹	2	18-1112-51
Tubing connector flangeless/M6 female ¹	2	18-1003-68
Tubing connector flangeless/M6 male ¹	2	18-1017-98
Union 1/16" female/M6 male ¹	6	18-1112-57
Union M6 female /1/16" male	5	18-3858-01
Union Luerlock female/M6 female	2	18-1027-12
HiTrap/HiPrep, 1/16" male connector for ÄKTAdesign	8	28-4010-81
Stop plug female, 1/16" ²	5	11-0004-64
Fingertight stop plug, 1/16" ³	5	11-0003-55

¹ One connector included in each HiTrap package

² Two, five, or seven female stop plugs included in HiTrap packages, depending on products

³ One fingertight stop plug is connected to the top of each HiTrap column

Related literature	Code No.
Antibody Purification Handbook	18-1037-46
Affinity Chromatography Handbook, Principles and Methods	18-1022-29
Convenient Protein Purification, HiTrap Column Guide	18-1129-81

www.gehealthcare.com/hitrap

GE Healthcare Bio-Sciences AB
Björkgatan 30
751 84 Uppsala
Sweden

Drop Design, HiTrap, HiPrep, ÄKTAdesign, ÄKTExplorer, Sepharose, PhastSystem, PhastGel and Superdex are trademarks of GE Healthcare companies. GE, imagination at work, and GE monogram are trademarks of General Electric Company.

All goods and services are sold subject to the terms and conditions of sale of the company within GE Healthcare that supplies them. General Electric Company reserves the right, subject to any regulatory and contractual approval, if required, to make changes in specifications and features shown herein, or discontinue the product described at any time without notice or obligation. Contact your local GE Healthcare representative for the most current information.

© 2006 General Electric Company – All rights reserved.

GE Healthcare Bio-Sciences AB, a General Electric Company.

GE Healthcare Europe GmbH
Munzinger Strasse 5, D-79111 Freiburg, Germany

GE Healthcare UK Ltd
Amersham Place, Little Chalfont, Buckinghamshire, HP7 9NA, UK

GE Healthcare Bio-Sciences Corp
800 Centennial Avenue, P.O. Box 1327, Piscataway, NJ 08855-1327, USA

GE Healthcare Bio-Sciences KK
Sanken Bldg. 3-25-1, Hyakunincho, Shinjuku-ku, Tokyo 169-0073, Japan

Asia Pacific Tel: +85 65 6 275 1830 Fax: +852 2811 5251 • Australasia Tel: +61 2 9899 0999 Fax: +61 2 9899 7511 • Austria Tel: 01/57606-1619 Fax: 01/57606-1627 • Belgium Tel: 0800 73 888 Fax: 03 272 1637 • Canada Tel: 800 463 5800 Fax: 800 567 1008 • Central, East, & South East Europe Tel: +43 1 982 3826 Fax: +43 1 985 8327 • Denmark Tel: 45 16 2400 Fax: 45 16 2424 • Finland & Baltics Tel: +358 (0)9 512 39 40 Fax: +358 (0)9 512 39 439 • France Tel: 01 69 35 67 00 Fax: 01 69 41 96 77 • Germany Tel: 0761/4903-490 Fax: 0761/4903-405 • Italy Tel: 02 27322 1 Fax: 02 27302 212 • Japan Tel: +81 3 5331 9336 Fax: +81 3 5331 9370 • Latin America Tel: +55 11 3933 7300 Fax: +55 11 3933 7304 • Middle East & Africa Tel: +30 210 9600 687 Fax: +30 210 9600 693 • Netherlands Tel: 0165 580 410 Fax: 0165 580 401 • Norway Tel: 815 65 555 Fax: 815 65 666 • Portugal Tel: 21 417 7035 Fax: 21 417 3184 • Russia & other C.I.S. & N.I.S Tel: +7 (095) 232 0250 Fax: +7 (095) 230 6377 • South East Asia Tel: 60 3 8024 2080 Fax: 60 3 8024 2090 • Spain Tel: 93 594 49 50 Fax: 93 594 49 55 • Sweden Tel: 018 612 1900 Fax: 018 612 1910 • Switzerland Tel: 0848 8028 12 Fax: 0848 8028 13 • UK Tel: 0800 616928 Fax: 0800 616927 • USA Tel: 800 526 3593 Fax: 877 295 8102

